

TX-9 Instrument Condenser Microphone

Type: Electret condenser

Frequency Response: 60 to 18,000Hz (see Figure 1)

Polar Pattern: Cardioid, rotationally symmetrical about microphone axis, uniform with frequency (see Figure 2)

Output Level (at 1,000Hz): Open circuit voltage: -70dB*
(0.32mV)*0dB=1V/μ bar

Output Impedance: 400Ω ± 30% (at 1,000Hz)

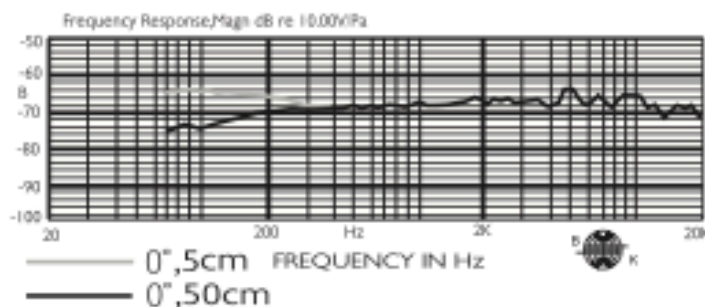


Figure 1


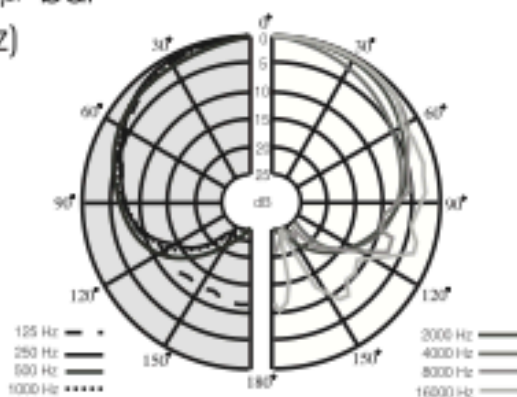


Figure 2

NOTE

1. If remote power is not available, install a UM-3(AA) 1.5V battery. Drive the screw located at the bottom of the mic body anti-clockwise and screw off the grill. Pull out the battery compartment. Install the battery with correct polarity and switch the power selector to "battery" position (see Figure 3).
2. Remember to remove the battery when do not use the microphone for long time.
3. The miking effect will vary according to the distance between sound source and the microphone (proximity effect)
4. Miking is a technique and an art. Always try to find your favorable miking method.
5. Avoid leaving the microphone in an environment where the temperature, humidity or both are extremely high.

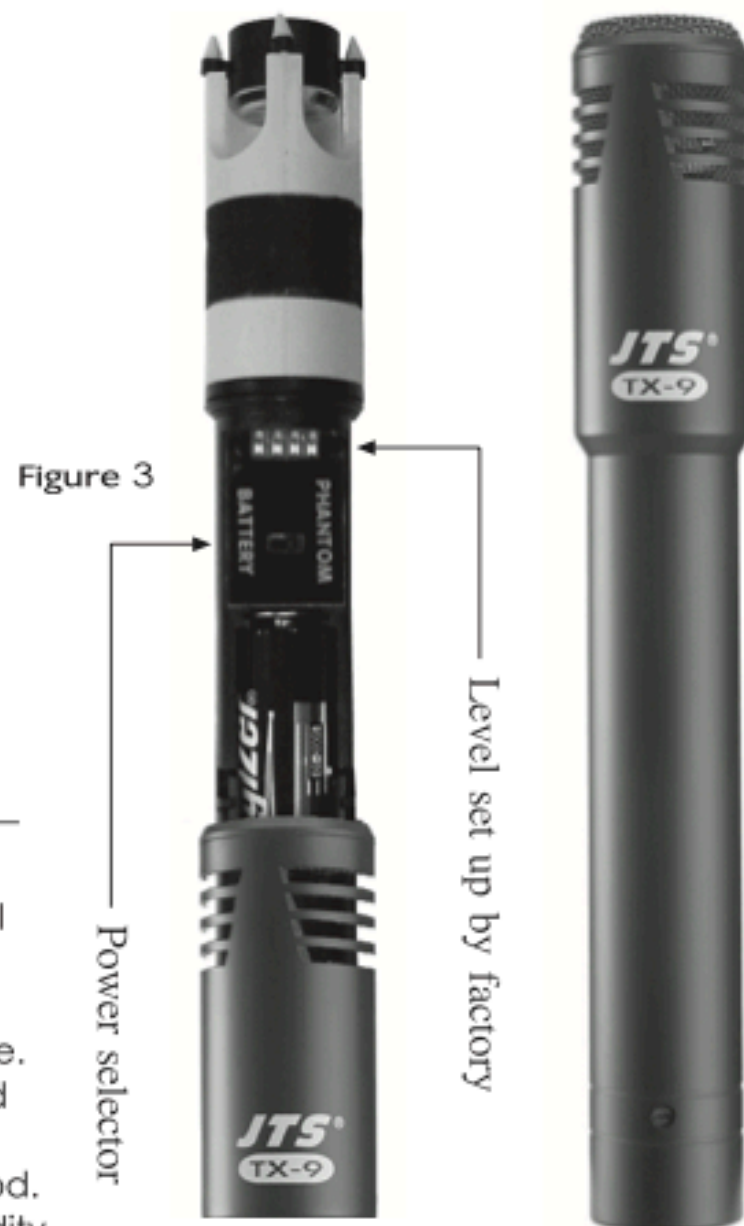

Instrument Condenser Microphone